

# Jones

## Medical Supply

### Home Oxygen & Medical Equipment

Thank you for allowing Jones Medical Supply to provide your home oxygen equipment. Below you will find step by step instructions on how to use your SimplyGo portable oxygen concentrator. **Important reminder; no smoking or open flames within 25 feet of you or the SimplyGo.**



- We've provided a 7ft cannula for you in the front pocket of the SimplyGo carrying case. A longer tubing and nasal cannula are also in the pocket to use when sleeping.
- After connecting the nasal cannula to the SimplyGo, press the power button **TWICE**.



- Your oxygen flow rate has been set by our staff as prescribed by your physician. This is represented by the number 1.0 - 6.0 on the screen of the SimplyGo.
- Next you will choose your delivery frequency by pressing the **“M”** on the SimplyGo. **CONTINUOUS FLOW, SLEEP MODE or PULSE MODE** are your three options. Typically you will use the **Pulse mode** when you're in a controlled resting environment. The Pulse mode determines oxygen delivery based on your breath, so concentrate on breathing through your nose. **Continuous flow** is more common if you are exerting yourself and can't take enough breathes to get the necessary oxygen while in Pulse mode. **Sleep mode** is a mixture of the two other settings but the machine ramps down the motor to ensure it does not affect your sleep. Please see the photos of the three modes on the reverse side of this document.

519-A South Brundidge St. \* Troy, AL 36081 \* 334-566-1002 \* fax 334-566-1003

[www.jonesmed.com](http://www.jonesmed.com)



# Jones

## Medical Supply


Home Oxygen & Medical Equipment

Continuous Flow

Pulse Mode

Sleep Mode

You must  
plug-in the SimplyGo when  
you enter SLEEP Mode

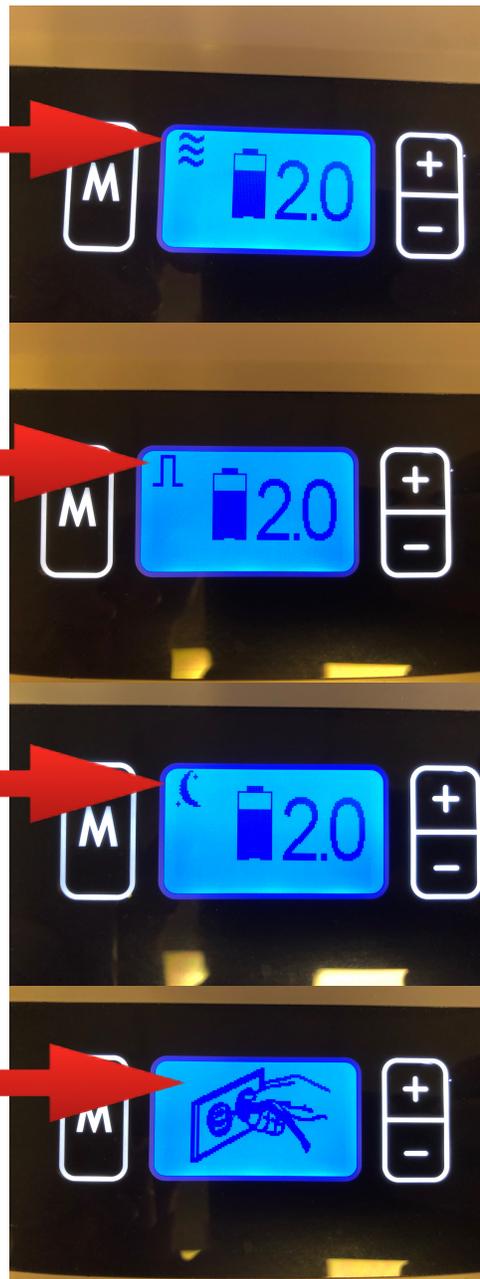

If you have any questions regarding this equipment, call our office anytime at 566-1002.

If it's after hours, a member of our staff is always available by phone.



519-A South Brundidge St. \* Troy, AL 36081 \* 334-566-1002 \* fax 334-566-1003

[www.jonesmed.com](http://www.jonesmed.com)

